

P/ INT COOPERATION TREAT

PCT

NOTIFICATION OF ELECTION

(PCT Rule 61.2)

From the INTERNATIONAL BUREAU

To:

Commissioner
 US Department of Commerce
 United States Patent and Trademark
 Office, PCT
 2011 South Clark Place Room
 CP2/5C24
 Arlington, VA 22202
 ETATS-UNIS D'AMERIQUE
 in its capacity as elected Office

Date of mailing (day/month/year) 04 April 2001 (04.04.01)	
International application No. PCT/GB00/02802	Applicant's or agent's file reference 23897
International filing date (day/month/year) 20 July 2000 (20.07.00)	Priority date (day/month/year) 20 July 1999 (20.07.99)
Applicant LOCK, Gary, Michael et al	

1. The designated Office is hereby notified of its election made:

☒ in the demand filed with the International Preliminary Examining Authority on:
 20 February 2001 (20.02.01)

☐ in a notice effecting later election filed with the International Bureau on:

2. The election ☒ was
☐ was not

made before the expiration of 19 months from the priority date or, where Rule 32 applies, within the time limit under Rule 32.2(b).

The International Bureau of WIPO 34, chemin des Colombettes 1211 Geneva 20, Switzerland Facsimile No.: (41-22) 740.14.35	Authorized officer S. Mafla Telephone No.: (41-22) 338.83.38
-----------------------------------------------------------------------------------------------------------------------------------	--------------------------------------------------------------------

(19) World Intellectual Property Organization
International Bureau




(43) International Publication Date
25 January 2001 (25.01.2001)

PCT

(10) International Publication Number
WO 01/05512 A1

- (51) International Patent Classification⁷: **B03C 5/02**
- (21) International Application Number: **PCT/GB00/02802**
- (22) International Filing Date: **20 July 2000 (20.07.2000)**
- (25) Filing Language: **English**
- (26) Publication Language: **English**
- (30) Priority Data:
9916850.2 20 July 1999 (20.07.1999) **GB**
- (71) Applicant (for all designated States except US): **UNIVERSITY OF WALES, BANGOR [GB/GB]**; College Road, Bangor, Gwynedd LL57 2DG (GB).
- (72) Inventors; and
- (75) Inventors/Applicants (for US only): **LOCK, Gary, Michael [GB/GB]**; 7 Hamilton Close, Lower Feltham, Feltham, Middlesex TW13 4PS (GB). **PETHIG, Ronald [GB/GB]**; Lleyn, Telford Road, Menai Bridge, Anglesey, Gwynedd LL59 5DT (GB).
- (74) Agent: **GALLAFENT, Richard, John**; Gallafent & Co, 9 Staple Inn, London WC1V 7QH (GB).
- (81) Designated States (national): **AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CR, CU, CZ, DE, DK, DM, DZ, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW.**
- (84) Designated States (regional): **ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).**
- Published:
— With international search report.
- For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: **DIELECTROPHORETIC APPARATUS & METHOD**

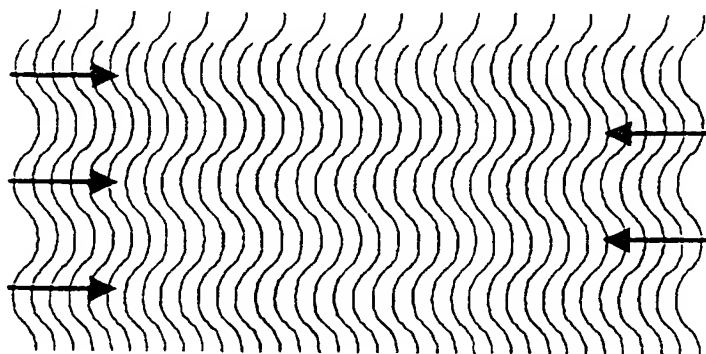

(57) Abstract: In a dielectrophoretic cell having an array of electrodes and means to apply electrical signals to the electrodes, the electrodes comprise a planar array of serpentine or zig-zag electrodes with their curvatures in register. The serpentine electrodes may be sinusoidal, half sinusoidal, or elongated "C" in shape; the positions of maximum curvature of each serpentine or zig-zag electrode may be arranged in linear alignment, or along a curve. The cell may be used for stationary or travelling wave dielectrophoresis. Particles travelling in opposite directions in travelling wave dielectrophoresis can do so without interference, allowing "traffic control". Particles can be characterised and separated, and particles at high concentrations, or particles of different types, can be handled.

WO 01/05512 A1

- 1 -

DIELECTROPHORETIC APPARATUS & METHOD

This invention relates to an apparatus and method of using the technique of dielectrophoresis, and relates
5 particularly to an arrangement for concentrating or diluting or transporting or separating or detecting or characterising particles.

The technique of dielectrophoresis (DEP) is described in
10 the book "Nanotechnology in Medicine and the Biosciences", Ed RRH Combs and D W Robinson, published by Gordon & Breach, Amsterdam, chapter 11 by Ronald Pethig, especially pages 88 to 93. Dielectrophoresis is the movement of particles in non-uniform electric fields. Unlike
15 electrophoresis, charges on the particle itself are not necessary for the effect to occur and AC rather than DC fields are employed.

When an electric field is applied to a system consisting of
20 particles suspended in a liquid medium, a dipole moment is usually induced in each particle as a result of electrical polarisations forming at the interfaces that define their structure. If the field is non-uniform, the particles

- 2 -

experience a translational force, known as a dielectrophoretic force, of magnitude and polarity dependent on the electrical properties of the particles and their surrounding medium. This force is also a
5 function of the magnitude and frequency of the applied electric field.

One application of the technique of DEP is described in WO 98/04355, British Technology Group, in which a
10 particle-containing liquid is caused to flow over a comb-like array of electrodes to which signals at different frequencies are applied; particles of different characteristics are urged preferentially towards or away from different DEP regions of the array,
15 so that the particles can be characterised. A flowing fluid is used.

The technique of travelling wave DEP is also described by Pethig, chapter 11, pages 93 to 97. One use of the
20 technique is described in WO 97/27933, University of Texas, in which a particle-containing liquid is caused to flow through a flat cell over an array of comb-like electrodes to which signals at different phases are applied so that by a combination of travelling wave DEP,
25 levitation, and field flow fractionation, separation and characterisation of the suspended particles is possible. A flowing fluid is used.

In conventional (i.e. using stationary rather than
30 travelling or rotating fields) DEP, it is also known to use castellated electrodes of the type illustrated in Figure 1, in which each electrode 10 comprises a straight linear backbone 12 having arranged alternately on opposite sides semi-circular protrusions 14.
35 Alternatively, the protrusions can be essentially square in shape. In an electrode array, the protrusions 14 on neighbouring electrodes can be aligned as illustrated,

- 3 -

or offset. The electrodes are used for conventional DEP, i.e. for non-travelling fields.

Throughout this specification, the term "particle" is
5 used to include biological cells, bacteria, viruses, parasitic microorganisms, DNA, proteins, biopolymers, non-biological particles, or any other particle which may be suspended in a liquid, in which a dielectrophoretic force can be induced. It also applies
10 to chemical compounds or gases dissolved or suspended in a liquid.

According to the invention, a dielectrophoretic cell comprising an array of elongated electrodes, and means
15 to apply at least one electrical signal to the electrodes, in which each electrode has a notional central axis along its direction of elongation, the electrode having one or more deflections from the notional central axis, and the electrodes in the array
20 being in register.

In the Shorter Oxford Dictionary, "deflection" is defined as "1. The action of bending down - bent condition; a bend or curve. 2. The action of turning,
25 or state of being turned from a straight line or regular course."

In one example, the electrodes are serpentine in shape with their curvatures in register. In another example,
30 the electrodes are zig-zag in shape with their points in register.

In one example, the electrodes in an array are all identical and parallel to each other. In another
35 example, the shape of the electrodes alters gradually along the array.

- 4 -

Also according to the invention, a dielectrophoretic method comprising placing a suspension of particles in a liquid in the vicinity of an array of electrodes, the array being defined and applying at least one electrical
5 signal to the array whereby particles are included in or excluded from regions of the electrodes corresponding to the maximum electrode curvatures. Alternatively, particles may be included in or excluded from regions of the electrodes corresponding to minimum electrode
10 curvatures.

Weiss and Thibodeaux in US Patent 4534856 describe an electrodynamic method for separating components such as grain and dust in agricultural by-products. This
15 separation of components is achieved by electrically charging them above a set of parallel electrodes that generate an electric travelling wave. This travelling wave is produced by energising the electrodes using a 60 Hz, 3-phase, high voltage generator and applied voltages
20 of up to 10,000 Volts and more. The forces acting on the component particles in US 4534856 are electrostatic in nature, involving the action of electric fields on charged bodies, rather than dielectrophoretic forces described in this present invention, where high
25 frequency signals in the range from around 1kHz to 100 MHz, and modest voltages in the range 1 - 20 Volts only, are employed.

WO 97/34689A1 describes apparatus for manipulating
30 particles along channels using dielectrophoresis. Figure 3 shows an electrode arrangement of the so-called interdigitated, castellated type. This is not a serpentine geometry. The castellations are designed to generate highly non-uniform field patterns that can
35 readily capture particles at the electrode castellation edges by positive dielectrophoretic forces. The effect of the castellation is not to produce the traffic

- 5 -

control or particle sieving effects which can be achieved by the apparatus and methods of the present invention.

- 5 WO 98/04355A1 describes a method for characterising how particles respond to dielectrophoretic forces over a wide frequency range using just one test. The particles are suspended in a chamber containing an array of electrode elements, as shown in Figure 3 of WO
- 10 98/04355A1. Each electrode is energised at a different electrical frequency, in order to generate a wide range of different dielectrophoretic forces. The dielectrophoretic response over this range is determined by inspecting how the particles are either attracted
- 15 towards or repelled from each electrode element. WO 98/04355A1 does not employ the travelling electric fields or the traffic control effects which can be achieved using the methods of the apparatus and present invention.
- 20
- US 5795457A describes a method for manipulating particles using stationary dielectrophoretic forces - travelling electric fields are not employed. Figure 1B(1)(a) in US 5795457A shows one of the electrode
- 25 arrangements that can be used, namely the so-called interdigitated, castellated, design. This is the same electrode geometry shown in Figure 3 of WO 97/34689A1, and, as stated above, this is not a serpentine geometry. The castellations are designed to generate highly non-
- 30 uniform field patterns that can readily capture particles at the electrode castellation edges by positive dielectrophoretic forces. The effect on the castellations is not to produce the traffic control or particle sieving effects which can be achieved by the
- 35 methods and apparatus of the present invention.

The invention will now be described by way of example

- 6 -

only with reference to the accompanying drawings in which:

Figure 2 indicates schematically a travelling wave
5 dielectrophoretic (TWD) system;

Figures 3A, B, C, D, E, F and G indicate various arrangements of TWD electrodes;

10 Figures 4A, B, C, D, E and F are successive photographs of an experimental separation of particles by TWD;

Figure 5 illustrates an array of TWD electrodes particularly suitable for separating two particles of
15 two or more different types;

Figure 6 illustrates schematically an alternative array of TWD electrodes;

20 Figure 7 illustrates an alternative arrangement of serpentine TWD electrodes;

Figure 8 shows a combination of conventional and serpentine TWD electrode arrays;
25

Figures 9A and 9B illustrate respectively an array of electrodes for static dielectrophoresis and appropriate electrical connections for the array; and

30 Figure 10 shows a variation of Figure 3A.

In Figure 2, a glass substrate 20 has on its upper surface an array 22 of serpentine electrodes, each of which is connected by a multiple connector 24 to a
35 signal generator 26. The substrate 20 can be covered by a protective cover 28 (conveniently a second glass substrate), the substrates being separated by a spacer,

- 7 -

not shown, to form a thin cell. A suitable spacer is a plastic strip. In a variation (not illustrated), the electrode array 22 may be fabricated on the protective cover 28.

5

The DEP cell is illuminated from below by a light source 30, and is viewed from above by an optical microscope/video recorder 32 connected to a display screen 36.

10

In use, a suspension of particles in a liquid is placed on a substrate 20 and the cover 28 put into place. The signal generator 26 is arranged to apply signals of different phases to the electrodes in the array 22. For example, the signal generator 26 may be a four-phase sinusoidal signal generator, connecting successive electrodes to signals of relative phase 0° , 90° , 180° and 270° , and then repeating the cycle across the whole array 22. As is well-known, such an array generates travelling wave DEP conditions. Alternatively, a stationary DEP force can be exerted on a particle by applying to adjacent electrodes in succession, sinusoidal signals in phase opposition (0° , 180° , 0° , 180° , etc.).

25

The DEP cell is illuminated by the light source 30 and is viewed on the screen 36. In transmission, particles will be seen as distinct areas, and their movement can be clearly seen on the screen.

30

It is to be noted that there need be no liquid flow through the cell.

Figures 3A to 3F illustrate six different serpentine electrode arrays. In each illustration, the arrows indicate the general directions of travel of the particles under the influence of the travelling wave

- 8 -

field, and also indicate the areas of travel within the field.

In Figure 3A, each electrode is sinusoidal in shape. In the Figure, three sinusoidal cycles are shown, the maxima and minima of each sinusoid being in register, i.e. in alignment. The arrows correspond to these cyclical maxima and minima, showing regions in which the particles travel. Three arrows point in one direction with two arrows, intermediate the three, pointing in the opposite direction; the arrows can be regarded as indicating channels of travel, and show that simultaneous travel in opposite directions is possible by different types of particle. The arrangement can be regarded as a traffic control system - particles travelling in opposite directions do not collide.

In known travelling wave DEP (TWD) arrangements using essentially straight, parallel electrodes, the general travelling wave force is the time averaged translational travelling force which occurs perpendicular to the electrodes.

In the serpentine electrode arrays according to the invention, the general travelling wave force is indicated by the arrows; the force "concentrates" the particles into certain regions and disperses them from other regions depending on electrode shape. Put another way, the particles are included in some regions and excluded from other regions of the travelling field.

Conditions can be selected so that particles of interest travel in one direction, and other particles travel in the opposite direction.

35

In Figure 3B, each electrode comprises a series of half sinusoids. All of the particles travelling from left to

- 9 -

right in Figure 3B can be regarded as travelling in separate bands in the direction of the arrows.

5 In Figure 3C, each electrode comprises an elongated "C" shape. All of the particles travelling from left to right in Figure 3C are excluded from the outer regions of the travelling field. This may be beneficial when there is a physical wall, at the edge of the field, thus avoiding bursting or other damage to the particles and
10 preventing loss in the process as particles stick to the adjacent wall. An additional effect is that "clogging" as a result is reduced, i.e. the tendency of multiple particles to stick together in a clump at a wall surface may be minimised.

15 In Figure 3D, each electrode has the form of a single half sinusoid connected between straight side arms. In this array, particles travel in correspondence with the curved part (mainly at maximum curvature). Particles
20 travelling from right to left are excluded from the areas corresponding to the central curved part of the array. The arrangement can be regarded as a one-way channel or a valve.

25 Figure 3E is similar to Figure 3B, except that each electrode is slightly offset from its neighbours so that the positions of maximum curvature of each electrode are arranged along parallel curves. The four channels
30 indicated by the arrows are curved, so the arrangement can be used to guide particles round corners of smaller radius than previously possible.

Figure 3F is similar to Figure 3A, except that the electrodes are zig-zag in shape instead of serpentine.

35 In Figure 3G, the electrodes are straight-line approximations to the sinusoids of Figure 3A, with each

- 10 -

full sinusoid being represented by five straight lines;
or the electrodes can be regarded as the zig-zags of
Figure 3F with flattened points. The arrows in the
channels now point in both possible directions of
5 travel, in contrast to the arrows in Figures 3A and 3F
because particles in the straight-line part at the
centre of the channels will remain in that region,
regardless of the direction of travel. Particles in the
'transition' region of electrodes, i.e. between the
10 channels, will move as illustrated in Figures 3A and 3F.
The arrangements of Figures 3A and 3F are therefore
preferable.

Inspection of the Figures 3A to 3F will show that a
15 common feature of all the electrodes is that they have
two or more different curvatures, either curves of
opposite direction, or a curved part and in some cases
straight portions. In another example, an electrode
array could comprise a series of C-shaped electrodes,
20 i.e. of a single curvature. Other shapes of serpentine
electrodes are also possible.

By selection of appropriate shapes of serpentine or zig-
zag electrode arrays, it is now therefore possible to
25 guide travelling particles into channels, to form them
into bands, to guide particles away from a mechanical
constraint on the liquid flow, such as apparatus walls,
and to guide them more easily round corners. Particles
can be included in a particular area of the DEP field,
30 or excluded from it. This allows particles to be
accurately positioned in a travelling field, thus easing
their detection. In addition, the technique can be used
to guide particles towards, e.g. an antibody-coated
object or surface.

35

Figure 4 illustrates particle movement using the
electrode array of Figure 3A and the general arrangement

- 11 -

of Figure 2. Sixty four sinusoidal electrodes in an array 22 were fabricated on a glass slide 20 by photolithography, and comprise a layer of chromium covered by a layer of gold. Each electrode is approximately 10 micrometers wide and the inter-electrode spacing is about 30 micrometers in the central channel regions. A culture of live yeast cells suspended in water was used, the cell concentration being 10.2 million cells per millilitre, and the conductivity of a suspension being 10.5 mS per metre. Prior to the experiment, the electrodes were soaked in ultra pure water for over an hour to help to clean them. In the experiment, it was found that by applying a stationary DEP signal at 150 kilohertz only levitation of the particles, as a result of a negative DEP force, occurs with no translational component.

In the experiment, a stationary DEP signal at a frequency of 150 kilohertz at 3 volts peak to peak was applied to all the electrodes in the array 22. The yeast cell suspension was then applied over the electrodes and a cover slip 28 placed on top. The 150 kilohertz signal caused the particles to levitate above the electrodes and minimises sticking of the yeast cells. After a few seconds, a 50 kilohertz, 3 volt peak-to-peak travelling wave DEP field was applied; the yeast cells immediately started to move along the travelling field and started to form into bands as can be seen from Figure 4A.

The large arrows indicate the general direction of movement of the cells, the small arrows indicate local movement of the cells as they are excluded from one channel and included in another, so that the cells form into bands. At the left hand side of the photographs, five channels are each given a channel number.

- 12 -

Figure 4B is a photograph taken about three seconds after Figure 4A; the cells can be seen to be moving to the right, and are more closely banded in channels 2 and 4, and are largely excluded from channels 1, 3 and 5.

5

Figure 4C was taken after the travelling wave field direction was changed. The cells are now travelling from right to left, and the bands can be seen moving out of channels 2 and 4 and into channels 3 and 5. Figure

10 4D was taken three or four seconds later, and the migration into bands is even more marked.

Figure 4E shows the bands a few seconds later, and illustrates that the cell movement is beginning to leave
15 a clear area in channels 3 and 5 as the cells are moved to the left.

Figure 4F is a photograph taken further along the channels to the left, showing that the bands are uniform
20 along the channels.

The small number of cells which are speckled over the electrodes are stuck to the glass and are not moving. At such high cell concentrations, some sticking of the
25 cells commonly occurs; this can be reduced by use of special coatings on the glass, or by using chemical agents such as surfactant or biochemical additives such as proteins (e.g. casein, denatured albumin) and using a polymeric material as a substrate, or placing a film of
30 polymeric material over a glass substrate.

The experimental results in Figure 4 show that particles can be formed into bands, along the direction of the travelling field and will move in those bands. At high
35 particle concentrations, travel in bands has been found to be particularly effective. The use of serpentine electrode geometries thus permits very high particle

- 13 -

concentrations to be handled more easily than has previously been possible using dielectrophoretic techniques.

- 5 If two particle populations are present which are of different properties, conditions can be selected so that they are caused to travel in opposite directions unhindered, allowing separation of the two types of particle. The technique works for low particle
10 concentrations but has also been found to be particularly effective when the aggregate particle concentration is very high, such as millions or tens of millions of particles per cubic centimetre, or even higher. Useful potential commercial applications may be
15 removing bacteria from saliva or stools; removing stem cells, foetal cells or cancer cells from blood; or removing meningital viruses from spinal fluid. In at least some of these cases, the numbers of particles to be removed may be very small compared to the numbers of
20 particles present, so the ability to work with high particle concentrations enables separation to be effected on a practical timescale.

- Experiments have been completed with human blood cells
25 using a similar electrode arrangement to those shown in Figures 3A and 4. The electrodes used were $8\mu\text{m}$ wide with $17\mu\text{m}$ inter-electrode spacing in the central channel regions. Experiments were completed at very high cell concentrations with a dilution of 10 times of whole
30 blood, a concentration of approximately 5×10^8 cells per millilitre (I.e. 500 million cells per cubic centimetre). Multi-phased signals were connected to the electrodes and the blood cells moved with TWD forces. A dilution of 20 times whole blood (I.e. a concentration
35 of approximately 2.5×10^8 cells per millilitre) was found to be preferable where separation rather than just the movement of particles is desired, particularly where

- 14 -

there is a large disparity in concentration between the cells to be separated. Disparity between cell concentrations was considerable, there being approximately 700 red blood cells for every white cell.

5

A particularly useful application of the serpentine electrode design involves the technique of signal superposition disclosed in UK Patent Application 9916848.6 and the International application based thereon and filed simultaneously with this application.

10

In one experiment, a 6 millilitre sample of human whole blood was collected in a lithium heparin tube, and within one hour was diluted 40 times in a phosphate-buffered saline solution containing sucrose, glucose, heparin and calcium chloride, to give a final suspension conductivity of 15 mS/m. The serpentine electrodes were energised with a 20 kHz, 0.6 Vrms stationary DEP signal so as to levitate the blood cells above the electrode plane when they were introduced into the test chamber. This DEP signal was then removed and two TWD signals were applied to the electrodes, one comprising a 50 kHz, 0.32 Vrms forward travelling wave and the other a 400 kHz, 0.64 Vrms reverse travelling wave. The majority of the blood cells moved rapidly along channels 3 and 5 similar to the case shown in Figure 4f, principally under the action of the 50 kHz signal. A small number, of the order 5% or less of the total number, of the blood cells were found to be trapped on the electrodes or to move slowly along channels 2 and 4 similar to the case shown in Figure 4a. Microscopic inspection, using a x40 objective, indicated that approximately 20-25 red blood cells were trapped or moving in channels 2 and 4 for every white blood cell. On re-applying the 20 kHz stationary DEP signal, the trapped red blood cells were directed into channels 3 and 5 and the largest of the white cells were released and moved along channels 2 and

35

- 15 -

4. These cells appeared mainly to be neutrophils, and moved along channels 2 and 4 at a speed of the order 15 microns per second. On reducing the frequency of the reverse TWD signal from 400 kHz down to 150 kHz, the smaller white blood cells were released from the electrodes and travelled along channels 2 and 4. This cell separation process for dilute blood has been repeated for different levels of blood dilution and suspending medium composition, and it can be appreciated that in each case the specific frequency and voltage values cited above for the superimposed DEP and TWD signals were adjusted to achieve the results described above.

15 Another valuable attribute of the serpentine electrode design is that it can be used in a sieving action to increase cell separation efficiency. This is achieved through a cycle of operations in which, after collecting the separated sub-population (target) cells, the main TWD signal is reversed so as to sieve out any of the target cells that may have been swept along with the main bulk of cells along channels 3 and 5. On sweeping these bulk cells in the reverse direction along channels 2 and 4, target cells that may have escaped the first separation process have the opportunity to be separated and to travel along channels 3 and 5. This process can be repeated the required number of times to achieve the desired efficiency for target cell recovery and purity of separation.

30

In the paper "Electromanipulation and separation of cells using travelling electric fields", J. Phys. D: Appln. Phys, 29, pages 2198-2203 (1996), Talary et al describe the separation of viable and non-viable yeast cells using TWD electrodes. The yeast cells were of the same order of size as blood cells and concentrations of approximately 1×10^4 cells per ml were subjected to TWD

- 16 -

forces using conventional electrodes of width $10\mu\text{m}$ and inter-electrode spacing of $10\mu\text{m}$. From the figures included in the publication, it can be appreciated that concentrations of the order 1×10^4 cells per ml represents close to the upper limit for the efficient manipulation and separation of cells using TWD with conventional electrode arrangements. This can be compared to the cell concentration of 2.5×10^8 cells per ml used with serpentine electrodes of the arrangement in Figure 3a, representing an increase of 25,000 times more cells per ml. Furthermore, in the publication by Talary et al, similar ratios of differing cell types (i.e. viable and non-viable yeast) were manipulated, where, as in the manipulation of whole blood cells using serpentine TWD electrodes, the ratio of red blood cells to white blood cells was in the order of 700:1 (a considerably more complex separation). Thus by means of this invention, considerably greater particle concentrations and greater particle type disparities can be handled, and the particles separated.

By means of the arrangement of the invention, low concentration of particles may also be handled and the particles manipulated, characterised and separated with increased levels of control compared to the application of straight parallel TWD electrodes. The invention may be applied to all ranges of particle concentration to effect, although in application its benefits may be most marked when handling high concentrations.

The inventive technique also overcomes a previous disadvantage of DEP in that particles travelling along a travelling field can tend to drift - the "focussing effect" achieved by the present invention minimises such drifting. Movement under a DEP field can now be distinguished from hydrodynamic fluid flow, which can cause comparatively substantial drifting. Hydrodynamic

- 17 -

fluid flow can be induced by heating effects caused by the electric fields.

Figure 5 illustrates an electrode arrangement for
5 separation of differing types of particle of different properties and different concentration. Conditions are selected so that the particles respond to the same travelling field by travelling in opposite directions; this can be achieved by changing, e.g. the properties of
10 the applied voltage signals, or the permittivity or electrical conductivity of the suspending liquid, or changing the temperature or even adding a chemical to the suspending liquid.

15 As will be seen from Figure 5, the electrodes at the upper part of the Figure are in the form of two cycles of a sinusoidal curve in register, but at the lower part of the Figure, the electrodes are in the form of two cycles separated by an almost straight part, the
20 electrode shape gradually changing from one to the other.

In operation, the sample suspension can be introduced on to the lower part of the electrode array or placed
25 directly on the whole electrode array. Particles of the higher concentration are arranged to move towards the top of the Figure in the central channel, while particles of the lower concentration are caused to move downwards along the two outer channels and are caused to
30 diverge away from the central area of the array.

In practice, the particles of high concentration may trap some of the particles of low concentration and carry them upwards. This is opposite to the effect of
35 the travelling wave DEP on the low concentration particles, and eventually they may free themselves and move into the two outer channels as required - a

- 18 -

substantial length of the central channel maximises this possibility, for example 0.5 to 5 cm. To further assist this escape from trapping, the travelling wave field may be intermittently switched off, allowing the particles
5 to disperse out of their band a little, and therefore assisting the lower concentration particles to escape. The same "sifting" effect can be achieved by intermittently reversing the field direction. This "sifting" effect is especially useful when working with
10 particles which tend to clot together, such as blood cells.

The Figure 5 arrangement may have application, for example, in separating organisms such as salmonella from
15 native E-coli and bacteroids in a sample of stool or separating cancer cells from blood. Cell separation using this sifting effect can also be achieved using other serpentine electrode geometries such as that of Figure 3A or 3B.

20 When there is a requirement to separate or concentrate or dilute one type or more of particle in a volume of liquid and to discard a second type of particle, the arrangement of Figure 6 can be used. The electrodes are
25 shown as thick lines, straight or curved, but each electrode is in fact a serpentine electrode such as that illustrated in Figure 3A.

The serpentine electrodes are arranged in two areas; a
30 central area A, in which each serpentine electrode has a straight axis, and the axes are parallel and transverse to the Figure - as indicated in the magnified view - and an outer area B in which the axes of the serpentine electrodes are "U" shaped. The outer area B therefore
35 has two side arms B1, B2 in which the electrode axes are straight, and a central connecting part B3 in which the electrode axes are curved.

- 19 -

The suspension of the mixture of particles is placed in contact with electrodes in both areas A and B, and the separation takes place in three stages:

- 5 1. Signals are applied to the electrodes in central area A so that particles of a first desired type travel downwards in the Figure and collect at the lower edge of the central electrode area, and particles of the second type travel upwards and
10 move over the outer electrode area B. By selection of appropriate electrode shape, the particles travel in opposite directions along different channels.
- 15 2. Signals are disconnected from the electrodes in the central area A, and applied to the outer area B so that particles of the desired type travel inwards to the inner area A, and particles of the other type travel outwards and off the edges of area B
20 and are discarded.
3. Signals to area B are disconnected and area A is reconnected, so that the desired particle type moves downwards and is collected at the bottom of
25 the central area.

In a variation, a multi-layer fabrication technique is used, and the inner and outer areas A and B are overlaid at their edges, separated by a thin insulating layer;
30 there is then no area in which particles may become trapped. For increased versatility of particle manipulation, different regions of electrode areas A and B may be controlled separately.

35 Once the technique of the invention has been applied, the separated or concentrated particle type of choice can be directed to a position at which they can be

- 20 -

analysed or characterised by a further DEP analysis, or by any other analysis technique such as optical, ultrasonic, electrical, magnetic, PLR, FISH, etc.

- 5 In all of the described arrangements, reference has been made to placing the liquid/particle suspension on the DEP electrode array. In a first alternative, the suspension may be placed on a substrate which carries the electrode array on its opposite face. In a second
10 alternative, the suspending liquid may first be placed on or adjacent the electrode array and the particles may be introduced afterwards; for example, in the Figure 5 array, the particles could be introduced in the central area at the bottom of the Figure. In a third
15 alternative, the suspension may be placed between two or more opposing electrode arrays fabricated on separate planar substrates or on a tubular substrate. However, none of arrangements depend on a fluid flow arrangement such as that used in conventional DEP. Fluid flow may
20 be used, but it is not a requirement.

- A further variation is shown in Figure 7. In all previous examples, the inter-electrode spacing indicated by s on Figure 7 has been constant, but in the
25 variation, the mark/space ratio w/s (where w is the width of the electrode) increases along the electrode array as shown.

- Figure 7B gives a side view of the serpentine electrodes
30 42, and indicates the forces on a particle p . The result of the varying mark/space ratio is that the levitation height of particles above the electrode array, indicated by a line L , increases. The forces on a particle P are shown, i.e. an upward levitation force
35 1 (the real part of the travelling wave DEP force), a translational force t_w (the imaginary part of the travelling wave DEP force), and gravity g . As the

- 21 -

particle moves to the right, the translational force decreases as a result of the increasing mark/space ratio; at the same time the levitation height of the particles increases, which results in a further
5 reduction of the translational force as the particle is further from the electrodes 42. At some point along line L, depending on particle size, the relative components of the dielectrophoretic force, the electric field strength, and electrode geometry, the
10 translational force will become zero, so no further travel occurs. Particles of different properties will therefore travel to different distances and reside in different positions. Particle separation is therefore possible.

15 In a variation, initial levitation is caused either by applying a static DEP field, or by applying a TWD field at a frequency at which the particles do not experience a translational force.

20 In a further variation, once particles have been separated into different regions as a result of utilising varied mark/space ratio electrodes, it is then desirable to be able to remove them selectively. Figure
25 8 shows an array of varied mark/space ratio electrodes 44, in this case conventional linear electrodes, closely adjacent an array of serpentine electrodes 46 of the type shown in Figure 3B (i.e. of constant mark/space ratio) for selective removal of particles. The arrays
30 of electrodes may either be fabricated using multi-layer techniques, or be fabricated on to opposing substrate faces. Utilising these two electrode arrays of different geometry in combination allows particle separation as a result of differing properties, and then
35 selective removal of the separated particles.

For example, particles may be introduced as indicated by

- 22 -

the arrow I. Particles of differing properties will travel different distances along the array of electrodes 44, and reside in different positions. These particles may then be removed along channels 'a' through to 'h' by the electrodes 46.

Numerous variants exist, using variations of serpentine, and combinations of serpentine and non-serpentine electrodes. Any of the electrode designs of Figures 3 and 5 may be used, or variants thereof. The choice of electrode geometries will depend on the choice of application. Changing the rate of change of the mark/space ratio of the electrodes can be beneficial depending on which particles are to be separated. For example, a linear or non-linear increase in mark/space ratio can be used. By using these variations, particles with very subtle differences may be separated and selectively removed.

All examples described above with reference to Figures 2 to 8 relate to travelling wave dielectrophoresis, although the electrode arrays may also be used to apply static DEP fields. Referring now to Figure 9, a set of serpentine electrodes suitable for static dielectrophoresis is shown. The electrodes 48 are "V" shaped and arranged in parallel pairs with the inter-electrode gap E being substantially greater than the inter-pair gap P. Each electrode in a pair projects on one side beyond the other electrode in that pair to facilitate connection to electrical connectors 50, 52 connected to opposite sides of a signal source 54.

Typically the electrodes 48 and connectors 50, 52 will be fabricated on a glass slide by photolithography, with the electrodes 48 being gold electrodes nominally 40 microns thick with an inter-electrode gap E also nominally 40 microns. Inter-pair gap P is nominally

- 23 -

200-1000 μ m. The slide carrying the electrodes will typically be formed into a cell with a spacer and a cover as in Figure 2, the chamber height being between 50 and 300 microns. However, for static
5 dielectrophoresis, as is well known, a flow system must be provided by particle suspension to cause movement as indicated by the arrow in Figure 9A. Such a flow system may be a mechanical system or flow may be caused by the well-known electrohydrodynamic effect on applying an
10 appropriate electrical signal to the electrode array.

If the signal applied to the electrodes 48 is of such a frequency that one type of particle in a suspension flowing through the cell experiences a strong negative
15 DEP force, according to known DEP principles, then such particles will be concentrated towards the regions of maximum curvature of the electrodes 48, while other particles flowing over the electrodes and experiencing a much weaker force, will be relatively unaffected.
20 Particle enrichment is therefore achieved.

The arrangement of Figure 3A refers to a traffic control system, where particles travelling in opposite directions will travel in the channel regions indicated
25 by the arrows without colliding. Figures 4A to 4F show electrodes of the arrangement of Figure 3A. These electrodes are of the form of very shallow or flat sinusoids. Alternatively, more pronounced or steep sinusoids may be used as shown in Figure 10. From
30 Figure 10, it is clearly seen that the result of steeper sinusoid electrodes is more defined transition regions, i.e. the regions between the channels. It is also clearly seen that the inter-electrode gaps are significantly greater in the centre of the channels than
35 they are in the transition regions.

The result of variations in the inter-electrode gaps

- 24 -

across the electrode array is regional levitation gradients. In the channel regions, particles will levitate higher, while in the transition regions, they will levitate to a lower height. In the centre of the
5 channels, the particles will levitate the highest, while in the centre of the transition region, they will be at their lowest levitation. The effects of this can be very beneficial for separations.

10 If a static DEP levitating field is applied, or a travelling DEP field where the translational TWD force for the particles is minimal, the particles will levitate above the electrodes and the substrate. This is beneficial for keeping the particles away from the
15 substrate and minimising particle sticking and clogging. In practice, it is therefore preferred to apply such a field prior to application of the particles. Applying such a field to the electrodes of Figure 10 and placing a solution of particles over them, after a few seconds
20 it can be seen that particles concentrate in the transition regions between the channels, with the particles moving out of the channel regions due to the regional levitation gradient. Particles feeling stronger levitation forces will move more quickly.
25 After the particles have concentrated in the transition regions, then applying a TWD field will result in particles which feel a strong TWD translational force moving into and along their respective channels. As a result of the regional levitation gradient, the channels
30 will be predominantly free of particles, allowing particles under strong translational TWD forces to travel freely along them unhindered, improving separation efficiency.

35 The regional levitation gradient has further application. Particles which feel a weak translational TWD force yet a strong levitation force will still move

- 25 -

along the dielectrophoretic cell, but the translational TWD force will be insufficient to overcome the levitation gradient. The particles will thus be restricted to movement within the transition region.

- 5 This can be used to keep these particles from the fast-moving particles experiencing a strong translational TWD force in the channels. This can be considered as a secondary traffic control system in that not only are particles which are travelling in opposite directions
10 prevented from interfering, but also fast and slow moving particles are segregated from each other. Different electrode geometries can be chosen either to enhance or to minimise this. As a further variation, this region levitation gradient can be used in
15 conjunction with fluid flow. A small amount of fluid flow may be applied in the channel to remove particles which experience very weak or no translational TWD force. The fluid flow may be applied from a source external to the dielectrophoretic cell, or, more
20 elegantly, a signal may be applied to the TWD electrodes which induces fluid flow, as is known. The result is that a weak fluid flow will have minimal effect on particles which experience strong TWD translational force, while particles feeling very weak or no
25 translational TWD forces will be moved along the dielectrophoretic cell within the transition regions, thus not disrupting particles moving in the channels. The movement of particles in such a manner with hydrodynamic fluid flow may be undertaken with any of
30 the electrode arrangements, and with or without TWD forces.

- When separations are undertaken on a suspension of particles with vastly different concentrations, it is
35 beneficial in aiding separation if conditions can be selected such that the particles are made to travel in opposite directions in a TWD field. In this case, it

- 26 -

may be beneficial to modify the electrodes of Figures 3A, 3F, 4 and 10. In the figures shown, the channels for particles travelling in opposing directions are of the same width. The width of the channels may be
5 changed to more closely reflect the disparity in concentrations of the particles travelling in them. This will make more efficient use of the electrode arrays in terms of particle movement and separation and may aid in allowing higher concentrations to be handled.

10

The examples have shown that serpentine or zig-zag electrodes according to the invention may be used with both stationary and travelling electric fields to both enrich and/or exclude and/or include particles from
15 areas of the electrode array and thus areas or regions of a chamber. This has many applications for characterising, separating, and/or identifying groups of, or individual particles. Both stationary fluid or fluid flow may be used in conjunction with the electrode
20 arrays, as may other external forces be used. Both positive and negative dielectrophoretic forces may be employed with the electrodes. Continuous separation of particles of very high concentrations is possible. By utilising these electrode arrays and predominantly
25 negative DEP forces, no cell trapping is used, and so relatively small electrode arrays may be used to handle very large particle concentrations and very large volumes, with enrichment of the sample resulting.

CLAIMS

1. A dielectrophoretic (DEP) cell in which particles
5 can be characterised, manipulated and separated
comprising an array of elongated electrodes, and means
to apply at least one electrical signal to the
electrodes, in which each electrode has a notional
central axis along its direction of elongation, the
10 electrode having one or more deflections from the
notional central axis, and the electrodes in the array
being in register.
2. A DEP cell according to Claim 1 in which the
15 electrodes are serpentine in shape.
3. A DEP cell according to Claim 2 in which the
serpentine electrodes are sinusoidal in shape.
- 20 4. A DEP cell according to Claim 2 in which the
serpentine electrodes are half sinusoidal in shape.
5. A DEP cell according to Claim 2 in which the
serpentine electrodes are of elongated "C" shape.
25
6. A DEP cell according to Claim 2 in which the
serpentine electrodes are single half sinusoids
connected between straight side arms.
- 30 7. A DEP cell according to Claim 1 in which the
electrodes are zig-zag in shape.
8. A DEP cell according to Claim 1 in which the
electrodes are straight line approximations to
35 sinusoids.
9. A DEP cell according to any one of Claims 2, 3, 7

- 28 -

or 8 in which the curvature of the deflections from the notional central axis on one side is different from the curvature of the deflections on the other side, whereby particle transport channels of different width are
5 provided.

10. A DEP cell according to any preceding Claim in which the positions of maximum curvature of each electrode are arranged in linear alignment.
10
11. A DEP cell according to any one of Claims 1 to 8 in which the positions of maximum curvature of each electrode are arranged in non-linear alignment.
- 15 12. A DEP cell according to Claim 11 in which the positions of maximum curvature of each electrode are arranged along a curve.
13. A DEP cell according to Claim 12 in which the
20 electrodes are serpentine and each comprises two sinusoids, and the positions of maximum curvature of the sinusoids are arranged along divergent curves.
14. A DEP cell according to any one of Claims 1 to 4
25 comprising a first central array of sinusoidal or half sinusoidal electrodes, the axes of the electrodes being straight and parallel, and a second outer array of sinusoidal or half sinusoidal electrodes, the axes of the electrodes being in the form of nested "U" shapes,
30 there being provided means to apply electrical signals of different phases independently to the first and second arrays.
15. A DEP cell according to any one of Claims 1 to 12
35 in which the inter-electrode spacing in the array varies along the array.

- 29 -

16. A DEP cell according to any one of Claims 1 to 12 in which the electrodes are arranged in pairs with the inter-electrode spacing being substantially greater than the inter-pair spacing.

5

17. A dielectrophoretic system comprising a DEP cell according to any one of Claims 1 to 15, at least a part of the cell being formed of transparent material; means to illuminate the cell; and means to receive
10 illumination transmitted through or reflected from the cell.

18. A dielectrophoretic method comprising placing a suspension of particles in a liquid in the vicinity of
15 an array of elongated electrodes in which each electrode has a notional central axis along its direction of elongation, the electrode having one or more deflections from the notional central axis, and applying at least one electrical signal to the array whereby particles are
20 included in or excluded from regions of the electrodes corresponding to the maximum or minimum electrode curvatures.

19. A method according to Claim 18 in which the
25 frequency of the electrical signals is selected to cause a negative dielectrophoretic response in a selected particle type in the suspension and there is further provided means to cause the liquid suspension to flow across the electrode array.

30

20. A method according to Claim 19 in which said means to cause the liquid suspension to flow is an electrical signal applied to the electrode array.

35 21. A method according to Claim 18 in which electrical signals at different phases are applied to the electrodes, whereby a travelling wave electric field is

- 30 -

generated which induces a travelling wave DEP force on said particles, the real part of said force levitating the particles, and the imaginary part thereof causing the particles to move into certain regions of the travelling field.

22. A method according to Claim 21 further comprising the initial step of applying to the electrode array an electrical signal whereby a static DEP field is generated so as to cause initial levitation of the particles.

23. A method according to Claim 21 further comprising the initial step of applying to the electrode array an electrical signal whereby a travelling wave electric field is generated at a frequency such that the particles are initially levitated but experience no translational force.

24. A method according to Claim 18 in which the suspension comprises a suspension of first and second types of particles, the concentrations of the types of particles differing by a factor of at least 1000, and in which the shape of the array of electrodes is selected so that the types of particles are separated.

25. A method according to Claim 24 in which the shape of the array of electrodes is selected to prevent particles from contacting a mechanical constraint on the liquid flow.



26. A method according to Claim 18 in which the concentration of the suspension of particles is greater than one million cells per millilitre.

27. A travelling wave dielectrophoretic cell substantially as hereinbefore described with reference

- 31 -

to any one of Figures 2, 3, 5, 6, 7, 8, 9 or 10 of the accompanying drawings.

Fig. 1

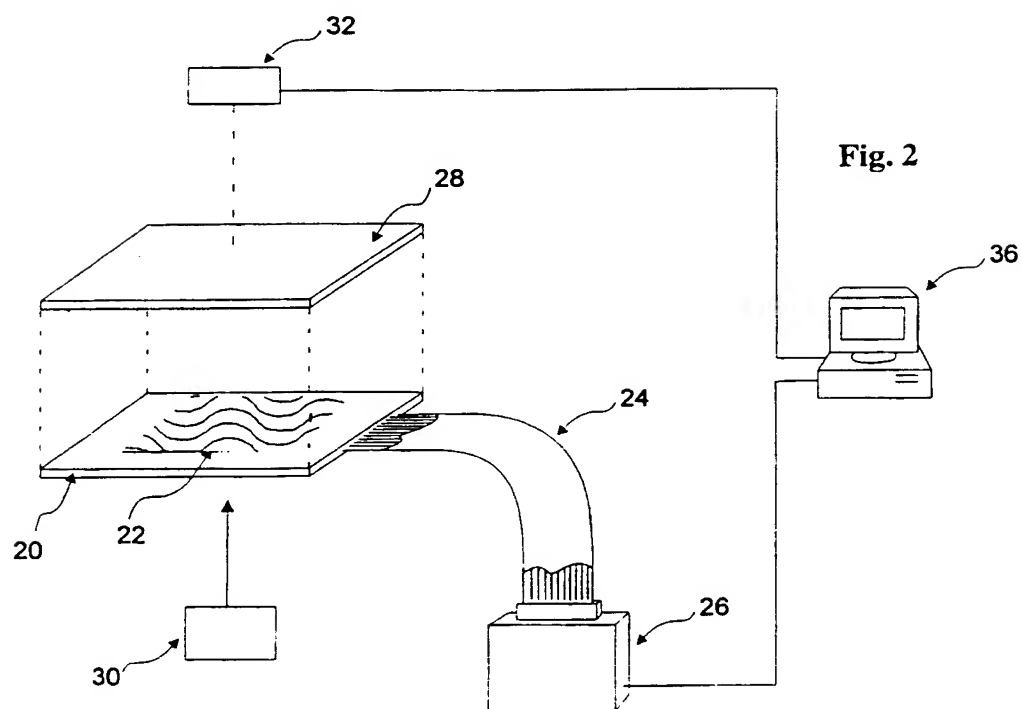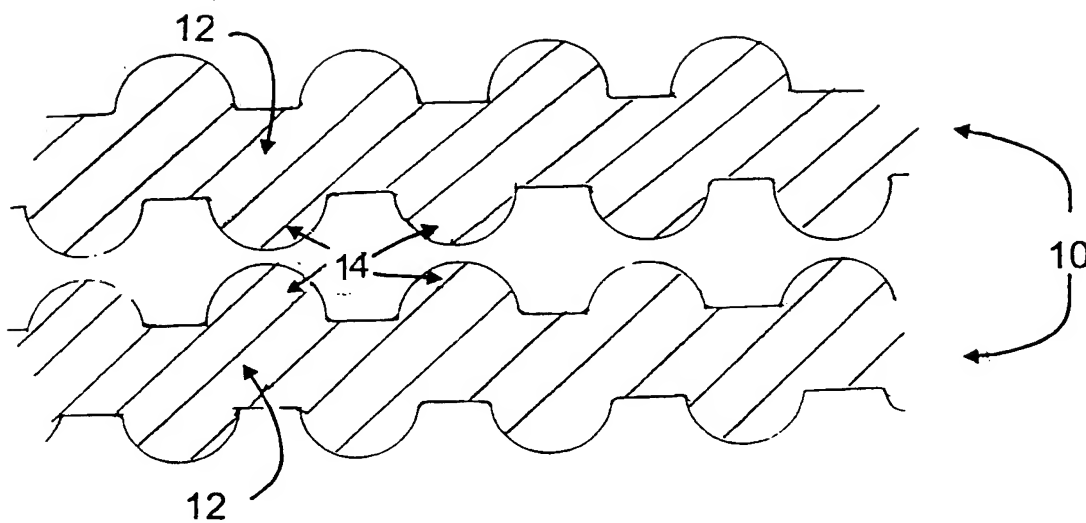

2/10

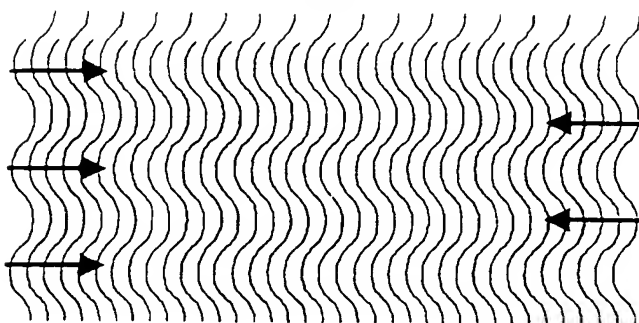


Fig. 3a

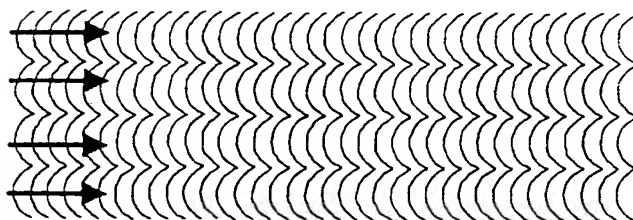


Fig. 3b

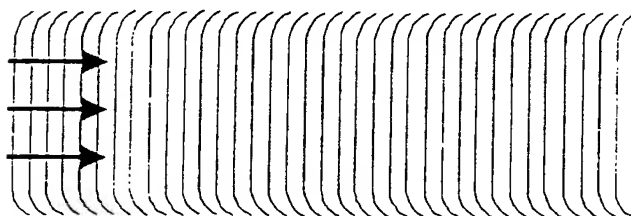


Fig. 3c

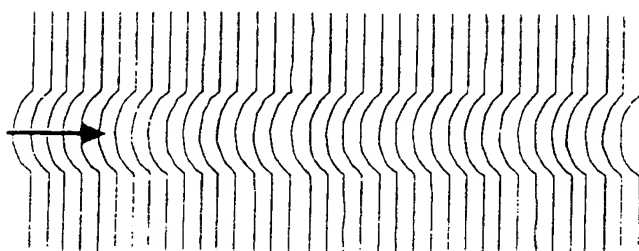


Fig. 3d

3/10

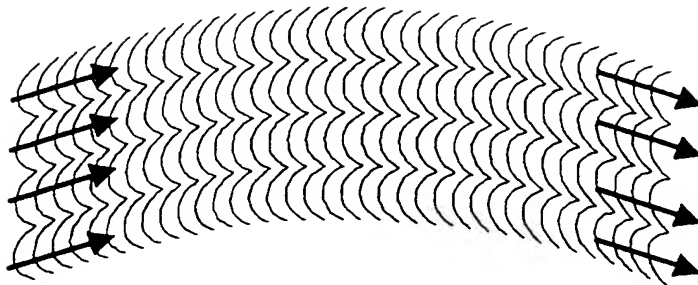


Fig. 3e

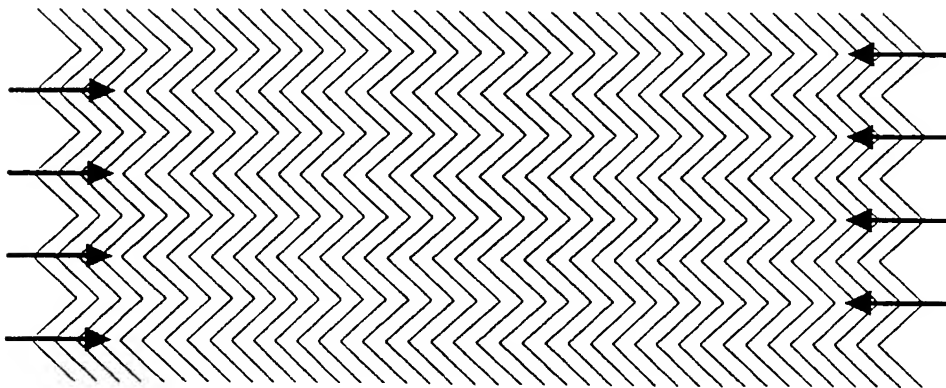


Fig. 3f

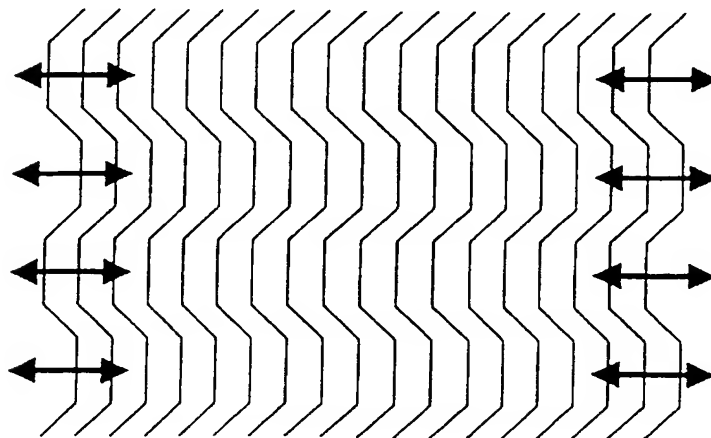


Fig. 3g

4/10

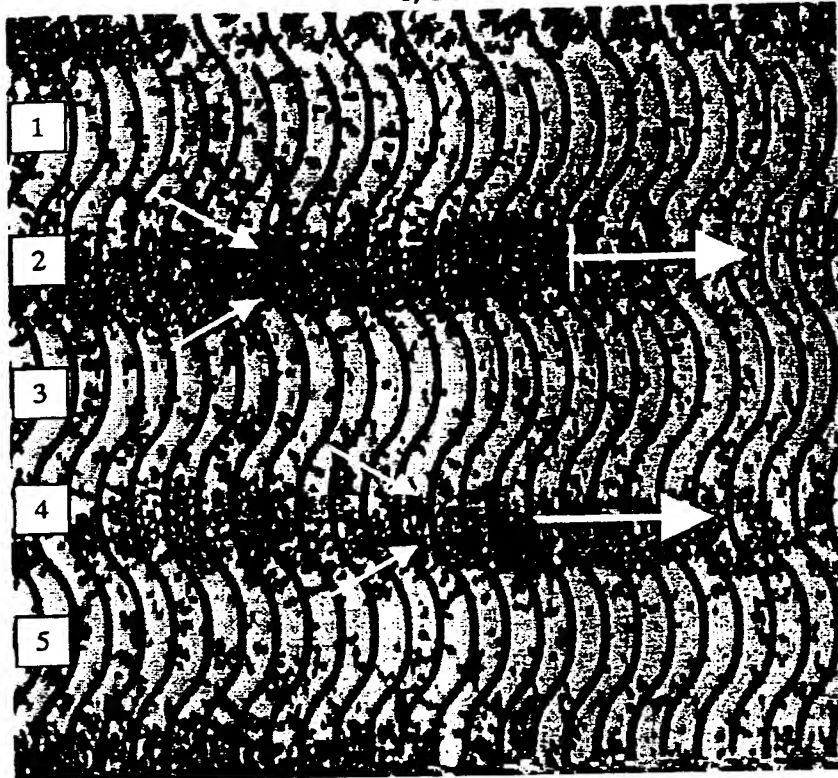


Fig. 4a

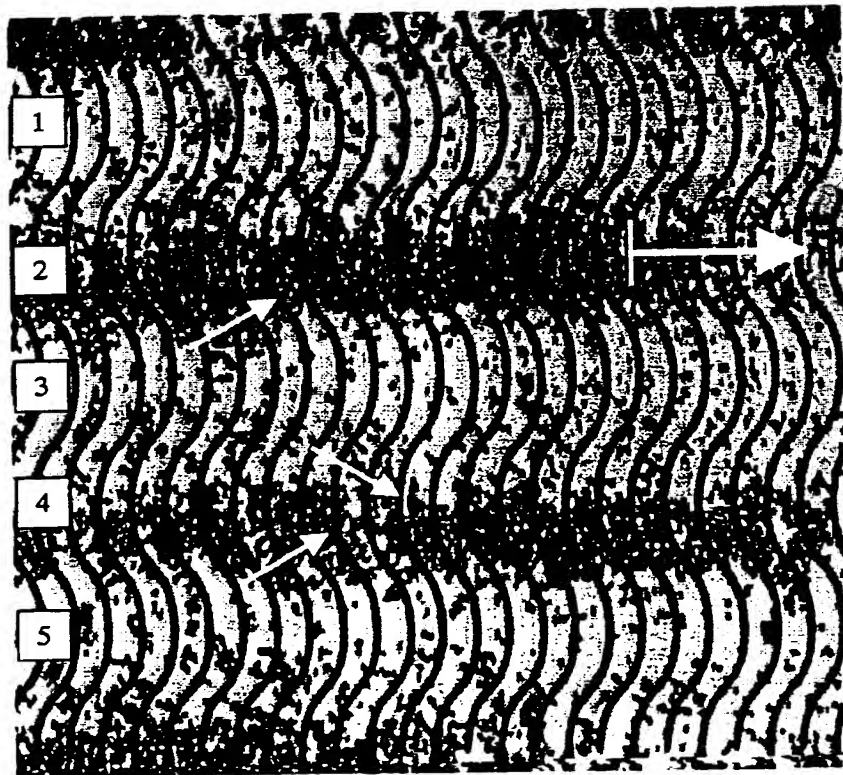


Fig. 4b

5/10

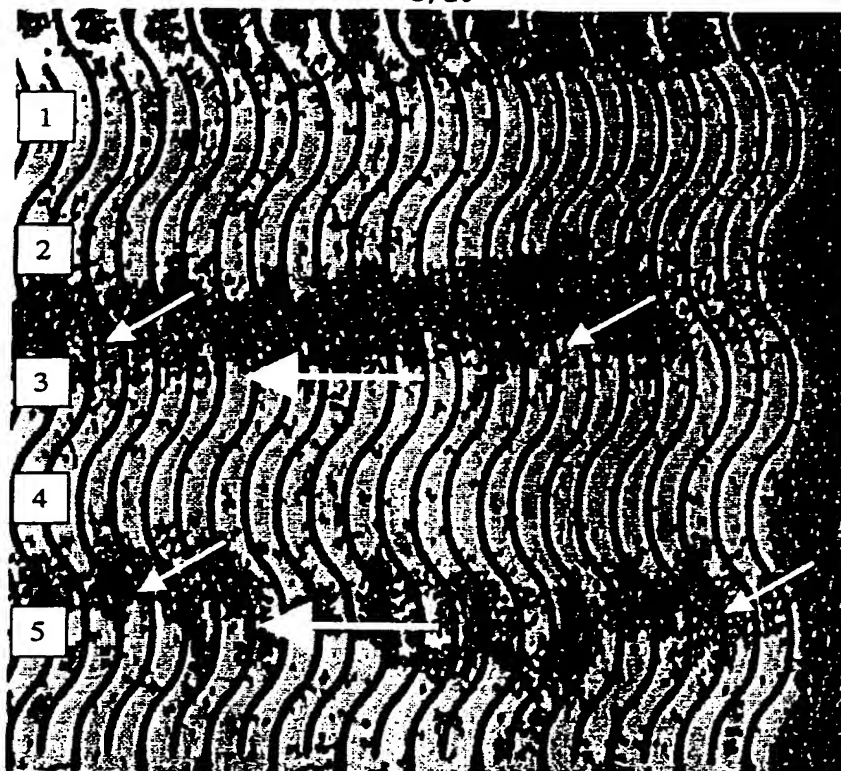


Fig. 4c

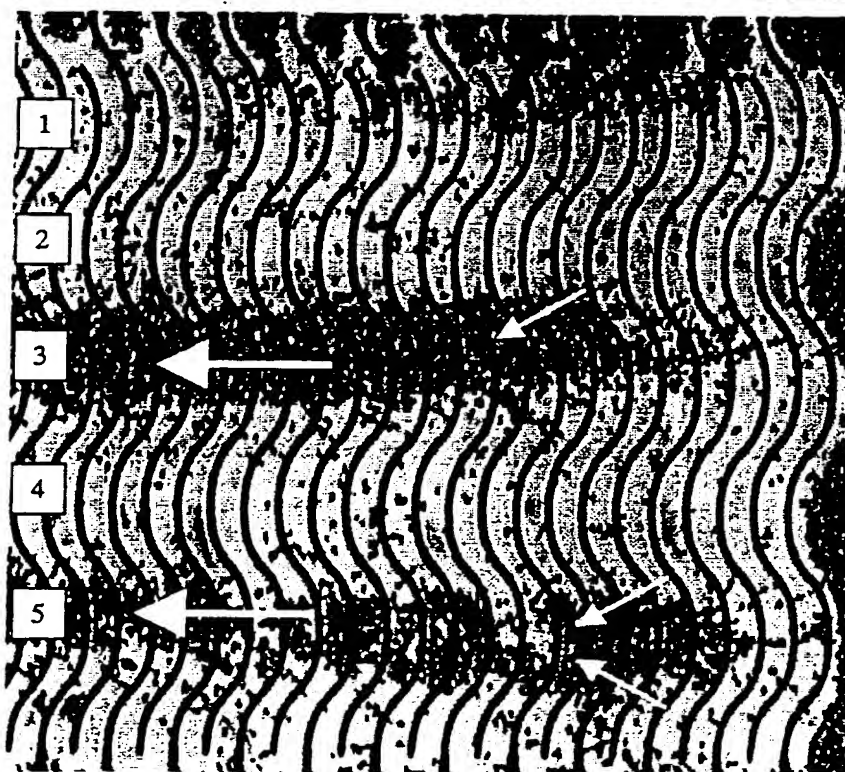


Fig. 4d

6/10

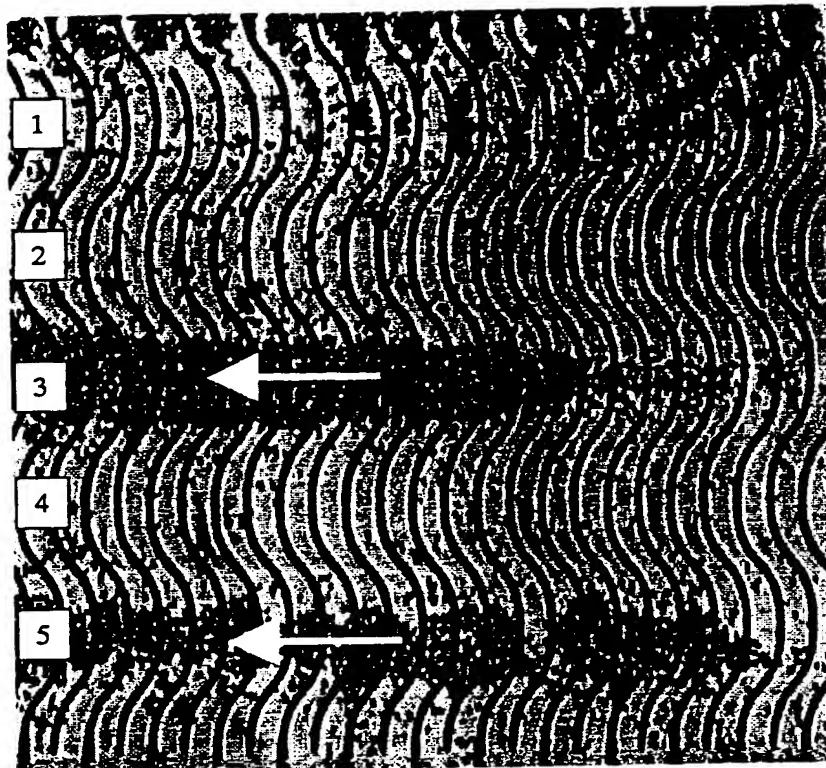


Fig. 4e

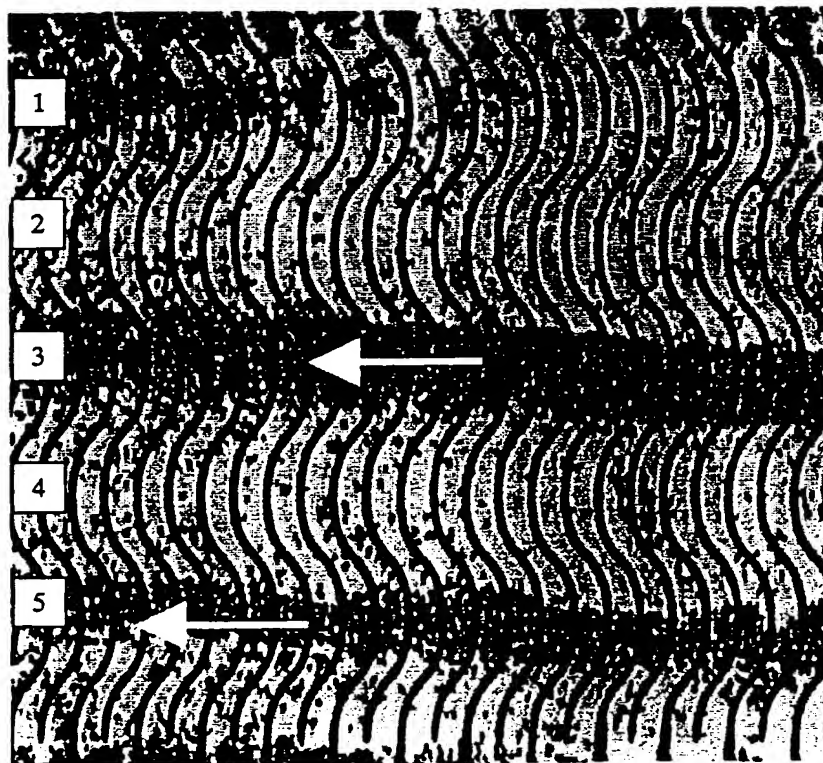


Fig. 4f

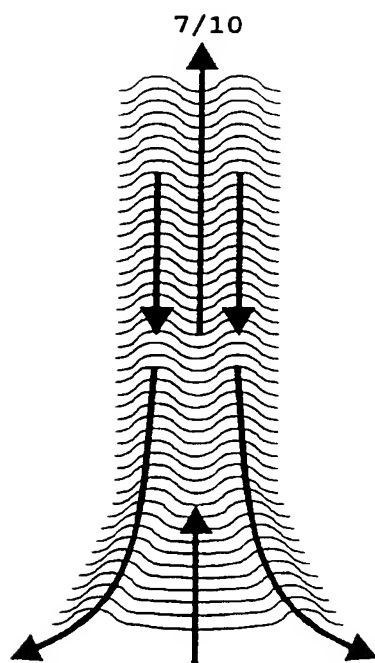


Fig. 5

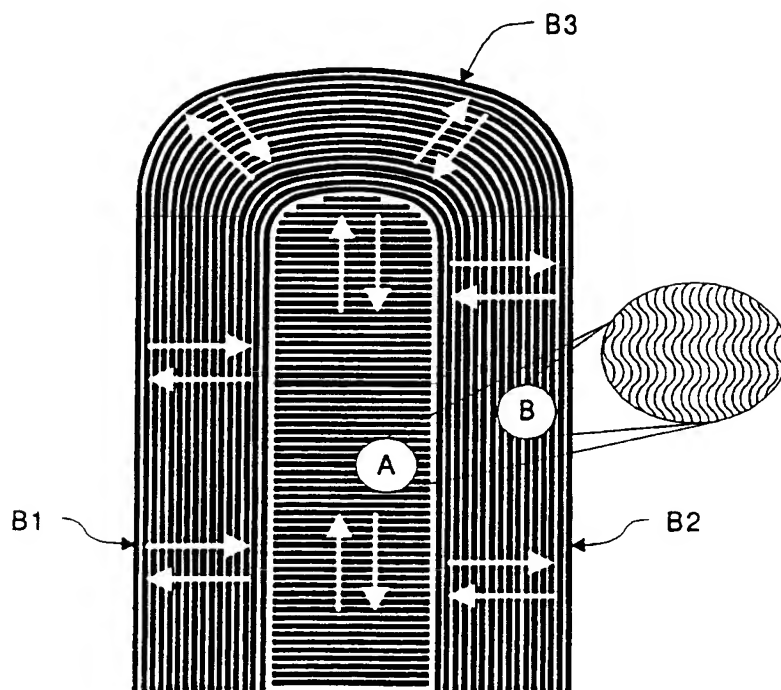


Fig. 6

8/10

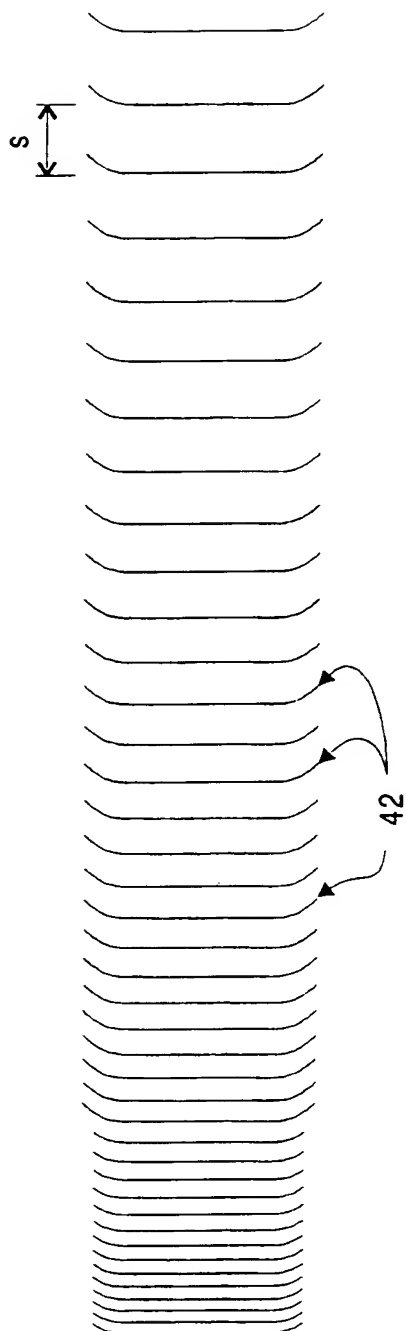


Fig. 7a

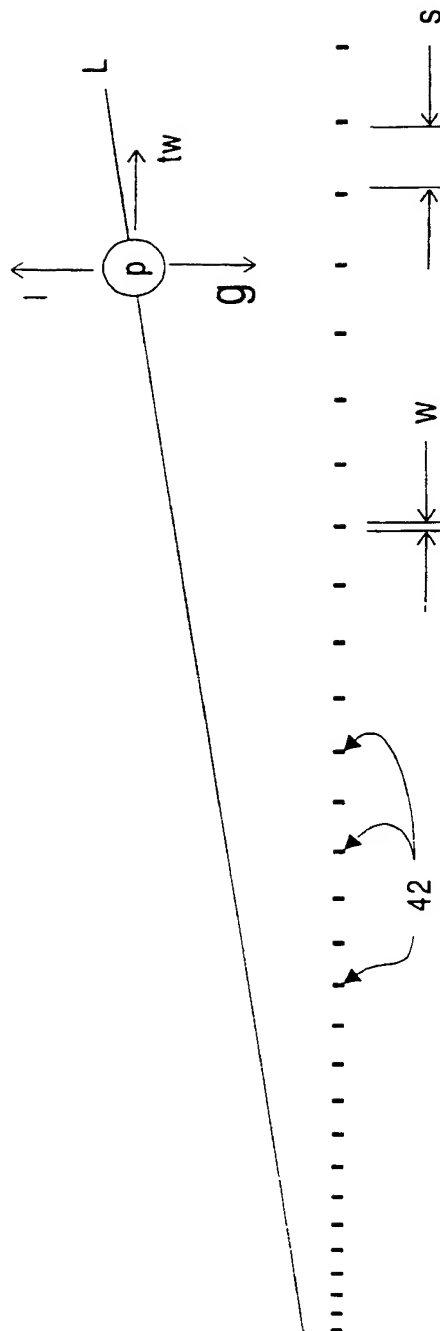


Fig. 7b

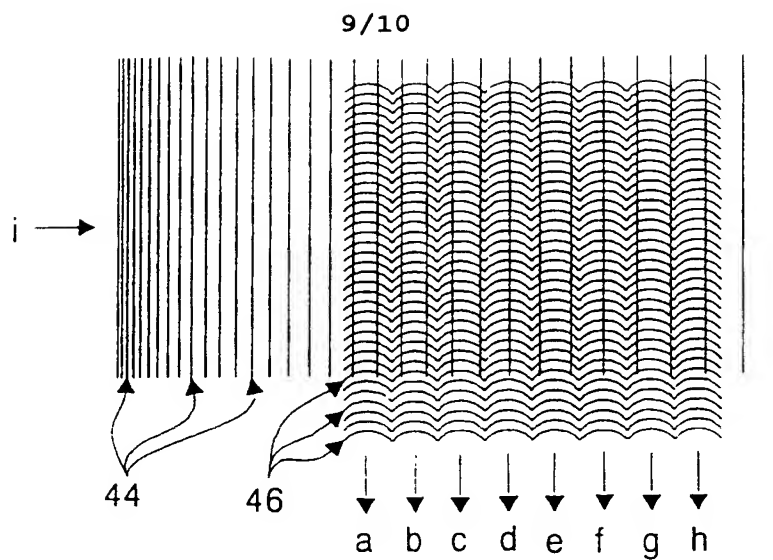


Fig. 8

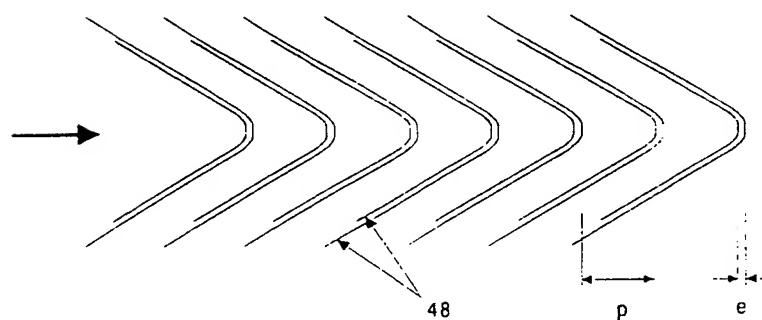


Fig. 9a

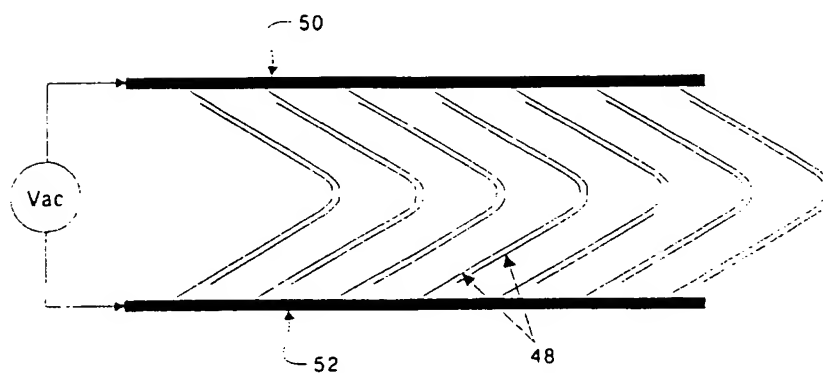


Fig. 9b

10/10

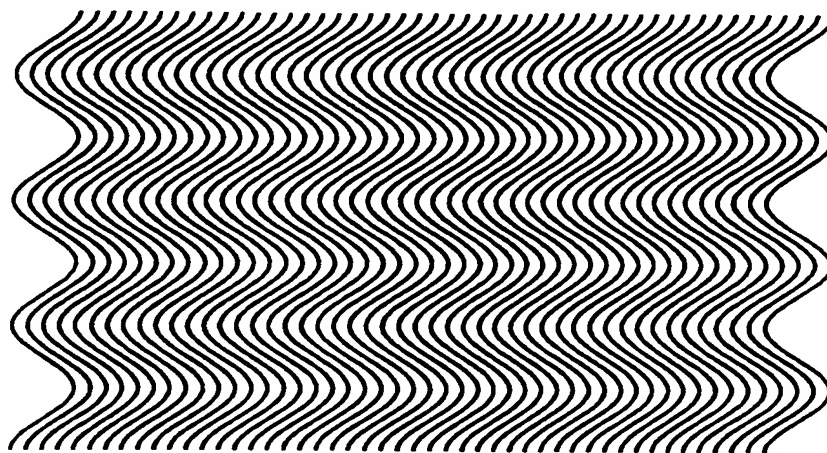


Fig. 10



PCT

WIPO

PCT

INTERNATIONAL PRELIMINARY EXAMINATION REPORT

(PCT Article 36 and Rule 70)

Applicant's or agent's file reference 23897	FOR FURTHER ACTION See Notification of Transmittal of International Preliminary Examination Report (Form PCT/IPEA/416)	
International application No. PCT/GB00/02802	International filing date (day/month/year) 20/07/2000	Priority date (day/month/year) 20/07/1999
International Patent Classification (IPC) or national classification and IPC B03C5/02		
Applicant UNIVERSITY OF WALES, BANGOR et al		
<p>1. This international preliminary examination report has been prepared by this International Preliminary Examining Authority and is transmitted to the applicant according to Article 36.</p> <p>2. This REPORT consists of a total of 5 sheets, including this cover sheet.</p> <p><input type="checkbox"/> This report is also accompanied by ANNEXES, i.e. sheets of the description, claims and/or drawings which have been amended and are the basis for this report and/or sheets containing rectifications made before this Authority (see Rule 70.16 and Section 607 of the Administrative Instructions under the PCT).</p> <p>These annexes consist of a total of sheets.</p>		
<p>3. This report contains indications relating to the following items:</p> <ul style="list-style-type: none">I <input checked="" type="checkbox"/> Basis of the reportII <input type="checkbox"/> PriorityIII <input type="checkbox"/> Non-establishment of opinion with regard to novelty, inventive step and industrial applicabilityIV <input type="checkbox"/> Lack of unity of inventionV <input checked="" type="checkbox"/> Reasoned statement under Article 35(2) with regard to novelty, inventive step or industrial applicability; citations and explanations supporting such statementVI <input type="checkbox"/> Certain documents citedVII <input checked="" type="checkbox"/> Certain defects in the international applicationVIII <input checked="" type="checkbox"/> Certain observations on the international application		
Date of submission of the demand 20/02/2001	Date of completion of this report 17.10.2001	
Name and mailing address of the international preliminary examining authority:  European Patent Office D-80298 Munich Tel. +49 89 2399 - 0 Tx: 523656 epmu d Fax: +49 89 2399 - 4465	Authorized officer Van Woensel, G Telephone No. +49 89 2399 2089 	

INTERNATIONAL PRELIMINARY EXAMINATION REPORT

International application No. PCT/GB00/02802

I. Basis of the report

1. With regard to the **elements** of the international application (*Replacement sheets which have been furnished to the receiving Office in response to an invitation under Article 14 are referred to in this report as "originally filed" and are not annexed to this report since they do not contain amendments (Rules 70.16 and 70.17)*):

Description, pages:

1-26 as originally filed

Claims, No.:

1-27 as originally filed

Drawings, sheets:

1/10-10/10 as originally filed

2. With regard to the **language**, all the elements marked above were available or furnished to this Authority in the language in which the international application was filed, unless otherwise indicated under this item.

These elements were available or furnished to this Authority in the following language: , which is:

- ☐ the language of a translation furnished for the purposes of the international search (under Rule 23.1(b)).
- ☐ the language of publication of the international application (under Rule 48.3(b)).
- ☐ the language of a translation furnished for the purposes of international preliminary examination (under Rule 55.2 and/or 55.3).

3. With regard to any **nucleotide and/or amino acid sequence** disclosed in the international application, the international preliminary examination was carried out on the basis of the sequence listing:

- ☐ contained in the international application in written form.
- ☐ filed together with the international application in computer readable form.
- ☐ furnished subsequently to this Authority in written form.
- ☐ furnished subsequently to this Authority in computer readable form.
- ☐ The statement that the subsequently furnished written sequence listing does not go beyond the disclosure in the international application as filed has been furnished.
- ☐ The statement that the information recorded in computer readable form is identical to the written sequence listing has been furnished.

4. The amendments have resulted in the cancellation of:

- ☐ the description, pages:
- ☐ the claims, Nos.:

**INTERNATIONAL PRELIMINARY
EXAMINATION REPORT**

International application No. PCT/GB00/02802

☐ the drawings, sheets:

5. ☐ This report has been established as if (some of) the amendments had not been made, since they have been considered to go beyond the disclosure as filed (Rule 70.2(c)):

(Any replacement sheet containing such amendments must be referred to under item 1 and annexed to this report.)

6. Additional observations, if necessary:

V. Reasoned statement under Article 35(2) with regard to novelty, inventive step or industrial applicability; citations and explanations supporting such statement

1. Statement

Novelty (N)	Yes:	Claims	
	No:	Claims	1-27
Inventive step (IS)	Yes:	Claims	
	No:	Claims	1-27
Industrial applicability (IA)	Yes:	Claims	1-27
	No:	Claims	

2. Citations and explanations
see separate sheet

VII. Certain defects in the international application

The following defects in the form or contents of the international application have been noted:
see separate sheet

VIII. Certain observations on the international application

The following observations on the clarity of the claims, description, and drawings or on the question whether the claims are fully supported by the description, are made:
see separate sheet

Ad V

1. Reference is made to the following documents:
D1: WO 98 04355 A
D2: WO 99 17883 A
D3: US-A-5 795 457
D4: WO 97 34689 A
2. The present application does not meet the requirements of Article 33(2) PCT, because the subject-matter of claims 1 and 18 is not new in the sense of Article 33(2) PCT.
 - 2.1 Document D2 discloses (see Fig. 3B; page 7, lines 10-15 and claims) a dielectrophoretic cell (and a dielectrophoretic method) in which particles can be characterised, manipulated and separated comprising an array of elongated electrodes, and means to apply at least one electrical signal to the electrodes, in which each electrode has a notional central axis along its direction of elongation, the electrode having one or more deflections from the notional central axis, and the electrodes in the array being in register.
Claims 1 and 18 are therefore not novel (Article 33(2) PCT).
 - 2.2 Also in view of D1 (see fig.2), D3 (see fig. 1B) and D4 (see fig.3), the present independent claims 1 and 18 lack novelty (Article 33(2) PCT).
The applicant describes the prior art known from these documents. However, the features which, according to the applicant, distinguish the present invention from D3 and D4, are not part of independent claims 1 or 18 since the electrodes of claim 1 are not limited to a serpentine shape.
 - 2.3 Independent apparatus claim 17 lacks novelty in view of D1, see page 5, lines 15-18.
3. The dependent claims are only allowable when related to a patentable independent claim.
In the present case, the dependent claims merely concern preferred embodiments of the invention which do not contain any features which meet the requirements of the PCT in respect of novelty or inventive step.

Ad VII

1. The features of the claims are not provided with reference signs placed in parentheses (Rule 6.2(b) PCT).
2. Claim 27 contains references to the description and the drawings. According to Rule 6.2(a) PCT, claims should not contain such references except where absolutely necessary, which is not the case here.
3. The independent claims are not in the two-part form in accordance with Rule 6.3(b) PCT, which in the present case would be appropriate, with those features known in combination from the prior art being placed in the preamble (Rule 6.3(b)(i) PCT) and with the remaining features being included in the characterising part (Rule 6.3(b)(ii) PCT).

Ad VIII

1. Although claims 1 and 17 have been drafted as separate independent claims, they appear to relate effectively to the same subject-matter and to differ from each other only with regard to the definition of the subject-matter for which protection is sought. The aforementioned claims therefore lack conciseness. Moreover, lack of clarity of the claims as a whole arises, since the plurality of independent claims makes it difficult, if not impossible, to determine the matter for which protection is sought, and places an undue burden on others seeking to establish the extent of the protection.

Hence, claims 1 and 17 do not meet the requirements of Article 6 PCT.

In order to overcome this objection, it would appear appropriate to file an amended set of claims defining the relevant subject-matter in terms of a single independent claim in each category followed by dependent claims covering features which are merely optional (Rule 6.4 PCT).